

**Progress in Metal Additive Manufacturing towards a Wide
Implementation in Dentistry**

Author

Hitzler, Leonhard, Alifui-Segbaya, Frank, Hall, Wayne, Oechsner, Andreas

Published

2016

Conference Title

Human Technologies: Engineering Applications in Sport and Health

Version

Version of Record (VoR)

Rights statement

© 2016 Queensland Sports Technology Cluster. The attached file is reproduced here in accordance with the copyright policy of the publisher. Please refer to the conference's website for access to the definitive, published version.

Downloaded from

<http://hdl.handle.net/10072/389809>

Link to published version

<http://www.qsportstechnology.com/>

Griffith Research Online

<https://research-repository.griffith.edu.au>

Progress in Metal Additive Manufacturing towards a Wide Implementation in Dentistry

Leonhard Hitzler^{1,a*}, Frank Alifui-Segbaya^{2,b}, Wayne Hall^{1,c} and Andreas Öchsner^{1,d}

¹ Griffith University, Griffith School of Engineering, Southport 4222, Australia

² Griffith University, Griffith School of Dentistry and Oral Health, Southport 4222, Australia

^aLeonhard.Hitzler@Griffithuni.edu.au, ^bF.Alifui-Segbaya@Griffith.edu.au, ^cW.Hall@Griffith.edu.au,

^dA.Oechsner@Griffith.edu.au

Keywords: Selective Laser Melting, Laser Polishing, Anisotropy, Biocompatibility, Dental Alloys

In recent years, the availability of high power lasers has enabled the full melting (FM) of raw materials, as in the case of selective laser melting (SLM), and hence, has overcome the necessity of a binder [1]. Thus, the FM allows the fabrication of parts with alloys suitable for dental applications. SLM eliminates many physical stages, required in the time-consuming investment casting process, by offering speed of the manufacturing process for bespoke metallic devices, such as denture frameworks and implant abutments [2-5]. The manufacturing process is solely based on dental and medical CAD data, which are designed on virtual anatomical patterns received from high-resolution dental scanners and CT, CBCT, MRI, photogrammetry, or surface scan data [6,7].

Cobalt-chromium (Co-Cr) and titanium alloys remain by far the most widely used alloys for affordable prosthodontics treatment. Documented studies show SLM fabricated parts possess adequate mechanical properties for clinical use [8-10]. In addition, available data indicates superior properties, in comparison to cast, for both tensile strength and fracture toughness [4,11-13]. These results show that a direct substitution of investment casting with SLM in the dental area is uncritical. In the assessment of biocompatibility, corrosion data, which forms an excellent adjunct to cytotoxicity studies, show that SLM fabricated samples have lower ion emission rates than cast ones (Fig. 1) [2,4]. Cytotoxicity studies also proved them safe, non-irritant and nontoxic on oral tissues and the body as a whole [14,15].

However, the design and dimensioning of components can be very challenging, as the layer-wise generation process results in anisotropic material properties, which are highly volatile to the manufacturing conditions [16]. For components designed close to the material limits, the dimensioning state has to account for the anisotropic properties, in both, the elastic and elasto-plastic range, including the stress-concentration effects of localized, inherent imperfections [17]. Currently, the surface roughness of 'as-built' SLM parts appears of insufficient quality for dental applications [18]. It is worth stating that the particular surface characteristics, and consequently their roughness, depend on the alignment and the positioning in the built space [19]. The choices available in post processing technologies to overcome the challenges of insufficient surface quality, while still maintaining the geometric flexibility in the built parts, are limited. On a positive note, recent studies have advanced from a proof of concept stage to polish the surface of SLM components with a laser; a process that could eliminate manual polishing altogether [20,21].

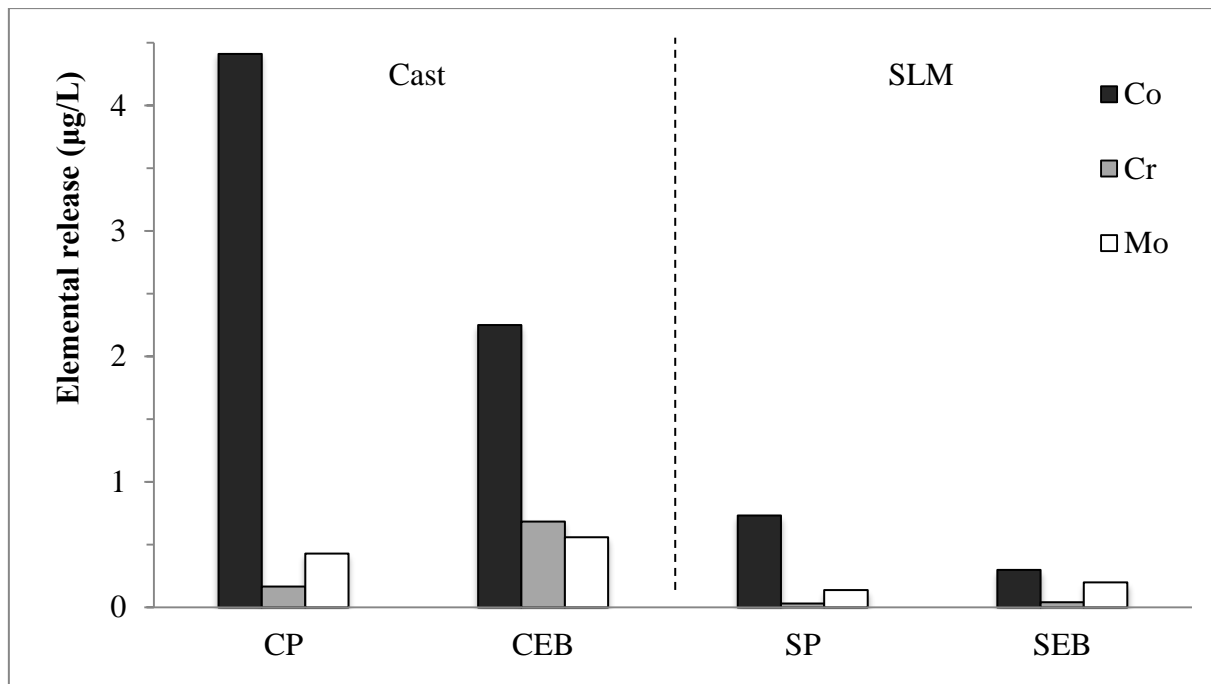


Figure 1: Elemental release of Co-Cr-Mo in artificial saliva after 42 days in accordance with ISO 10271 on: CP = cast and polished; CEB = cast and electro-brightened; SP = SLM-fabricated and polished; SEB = SLM-fabricated and electro-brightened; adopted from [4]

Conclusion

The SLM process, although high-priced to acquire, offers increased speed and flexibility in dental technology. Likewise, the SLM process, being controlled digitally, offers a standard method for the production of dental devices, which is likely to be much closer to the manufacturer's specifications than investment casting that is fraught with fabrication steps and operator variations. Nevertheless, further studies are required to understand the parameters that influence the physico-mechanical properties of SLM fabricated components.

References

- [1] P. Rochus, J.Y. Plessier, M. Van Elsen, J.P. Kruth, R. Carrus, T. Dormal, New applications of rapid prototyping and rapid manufacturing (RP/RM) technologies for space instrumentation. *Acta Astronaut* 61 (2007) 352-359.
- [2] F. Alifui-Segbaya, P. Foley, R.J. Williams, The corrosive effects of artificial saliva on cast and rapid manufacture-produced cobalt chromium alloys. *Rapid Prototyping Journal* 19 (2013) 95-99.
- [3] F. Alifui-Segbaya, J. Lewis, D. Eggbeer, R.J. Williams, In vitro corrosion analyses of heat treated cobalt-chromium alloys manufactured by direct metal laser sintering. *Rapid Prototyping Journal* 21 (2015) 111-116.
- [4] F. Alifui-Segbaya (2011) 'In vitro' tensile tests and corrosion analyses of a rapid manufacture-produced cobalt-chromium alloy compared to cast cobalt-chromium alloys. Thesis, Cardiff Metropolitan University, Cardiff
- [5] F. Alifui-Segbaya, R.J. Williams, The corrosion of electrobrightened and polished cast and rapid manufacture-produced cobalt chromium alloys. *The Dental Technician Journal* 64 (2011) 10-11.
- [6] R. Van Noort, *Introduction to Dental Materials*, 4 edn. Elsevier, Sydney, 2013.

- [7] Medical Models (2015) PDR Cardiff Metropolitan University. <http://pdronline.co.uk/surgical-and-prosthetic-design/medical-models>. Accessed 18 October 2015
- [8] F. Alifui-Segbaya, J. Evans, D. Eggbeer, R. George, Clinical relevance of laser-sintered cobalt-chromium alloys for prosthodontic treatment: a review. *Proc. of the Intl. Conf. on Progress in Additive Manufacturing*, pp 115-120, (2014)
- [9] D. Jevremovic, T. Puskar, B. Kosec, D. Vukelic, I. Budak, S. Aleksandrovic, D. Egbeer, R. Williams, The analysis of the mechanical properties of F75 Co-Cr alloy for use in selective laser melting (SLM) manufacturing of removable partial dentures (RPD). *Metalurgija* 51 (2012) 171-174.
- [10] A.R. Lapcevic, D.P. Jevremovic, T.M. Puskar, R.J. Williams, D. Eggbeer, Comparative analysis of structure and hardness of cast and direct metal laser sintering produced Co-Cr alloys used for dental devices. *Rapid Prototyping J* 22 (2016).
- [11] Y. Kajima, A. Takaichi, T. Nakamoto, T. Kimura, Y. Yogo, M. Ashida, H. Doi, N. Nomura, H. Takahashi, T. Hanawa, N. Wakabayashi, Fatigue strength of Co–Cr–Mo alloy clasps prepared by selective laser melting. *Journal of the Mechanical Behavior of Biomedical Materials* 59 (2016) 446-458.
- [12] A. Takaichi, Suyalatu, T. Nakamoto, N. Joko, N. Nomura, Y. Tsutsumi, S. Migita, H. Doi, S. Kurosu, A. Chiba, N. Wakabayashi, Y. Igarashi, T. Hanawa, Microstructures and mechanical properties of Co–29Cr–6Mo alloy fabricated by selective laser melting process for dental applications. *Journal of the Mechanical Behavior of Biomedical Materials* 21 (2013) 67-76.
- [13] L. Hitzler, J. Hirsch, J. Schanz, B. Heine, M. Merkel, W. Hall, A. Öchsner, Fracture toughness of selective laser melted AlSi10Mg. *P I Mech Eng L: J Mat* SUBMITTED (2017).
- [14] D. Jevremovic, V. Kojic, G. Bogdanovic, T. Puskar, D. Eggbeer, D. Thomas, R. Williams, A selective laser melted Co-Cr alloy used for the rapid manufacture of removable partial denture frameworks - initial screening of biocompatibility. *J Serb Chem Soc* 76 (2011) 43-52.
- [15] T. Puskar, A. Lapcevic, S. Arandjelovic, S. Radulovic, I. Budak, D. Vukelic, D. Jevremovic, Comparative study of cytotoxicity of direct metal laser sintered and cast Co-Cr-Mo dental alloy. *Metalurgija* 54 (2015) 481-484.
- [16] L. Hitzler, C. Janousch, J. Schanz, M. Merkel, B. Heine, F. Mack, W. Hall, A. Öchsner, Direction and location dependency of selective laser melted AlSi10Mg specimens. *J Mater Process Technol* 242 (2017) IN PRESS.
- [17] A. Öchsner, *Continuum Damage and Fracture Mechanics*. Springer, Singapur, 2016.
- [18] L. Hitzler, C. Janousch, J. Schanz, M. Merkel, F. Mack, A. Öchsner, Non-destructive evaluation of AlSi10Mg prismatic samples generated by Selective Laser Melting: Influence of manufacturing conditions. *Mat-wiss u Werkstofftech* 47 (2016) 564-581.
- [19] L. Hitzler, J. Hirsch, M. Merkel, W. Hall, A. Öchsner, Position dependent surface quality in Selective Laser Melting. *Mat-wiss u Werkstofftech* IN PRESS (2017).
- [20] J. Schanz, M. Hofele, L. Hitzler, M. Merkel, H. Riegel Laser polishing of additive manufactured AlSi10Mg parts with an oscillating laser beam. In: *Machining, Joining and Modifications of Advanced Materials*. Springer, Singapore, 2016, pp 159-169.
- [21] J. Schanz, M. Hofele, S. Ruck, T. Schubert, L. Hitzler, G. Schneider, M. Merkel, H. Riegel, Metallurgical Investigations of Laser Remelted Additively Manufactured AlSi10Mg Parts. *Mat-wiss u Werkstofftech* IN PRESS (2017).